



**EKOTEKS LABORATUVAR ve GÖZETİM
HİZMETLERİ A.Ş.**
Esenyurt Firuzköy Bulvarı No:29 34325 Avcılar
İstanbul/ TÜRKİYE



TEST REPORT
DENEY RAPORU

AB-0583-T

20027353

08-20

Customer name: NARKONTEKS TEKSTİL İHR İTH SAN VE TİC AŞ
Address: DOĞUŞ CAD 3/19 SOK NO:12 BUCA İZMİR
Buyer name: -
Contact Person: AYSUN AYHAN/BAŞAK BULUT/BURCU ASLAN
Order No: -
Article No: 9040
Name and identity of test item: White gown fabric.(White)
The date of receipt of test item: 06.08.2020
Re-submitted/re-confirmation date: -
Date of test: 06.08.2020-13.08.2020
Remarks: -
Sampling: The results given in this report belong to the received sample by vendor.
End-Use: -
Care Label: Not specified.
Number of pages of the report: 3

The Turkish Accreditation Agency (TURKAK) is signatory to the multilateral agreements of the European co-operation for the Accreditation (EA) and of the International Laboratory Accreditation (ILAC) for the Mutual recognition of test reports.

EKOTEKS LABORATUVAR ve GÖZETİM HİZMETLERİ A.Ş. accredited by TÜRKAK under registration number [AB-0583-T] for ISO 17025:2017 as test laboratory.

The test and/or measurement results, the uncertainties (if applicable) with confidence probability and test methods are given on the following pages which are part of this report.

Seal



Date
13.08.2020

Customer Representative
Zahide TAPAN

Head of Testing Laboratory
Sevim A. RAZAK
13.08.2020

This report shall not be reproduced other than in full except with the permission of the laboratory.
Testing reports without signature and seal are not valid.

EKOTEKS LABORATUVAR ve GÖZETİM
HİZMETLERİ A.Ş.


AB-0583-T

20027353

08-20

REQUIRED TESTS	RESULT	COMMENTS
PHYSICAL PROPERTIES TESTS		
Water Resistance (Impact Penetration)	P	
Water Permeability	P	
P: Pass F: Fail R: Refer to retailer technologist. Tests were as per AAMI PB70 guidelines.		

REMARK: Original samples are kept for 3 months and all technical records are kept for 5 years unless otherwise specified. If requested, measurement uncertainty will be reported. But unless otherwise specified, measurement uncertainty is not considered while stating compliance with specification or limit values. The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95 %. Tests marked (*) in this report are not included in the accreditation schedule.

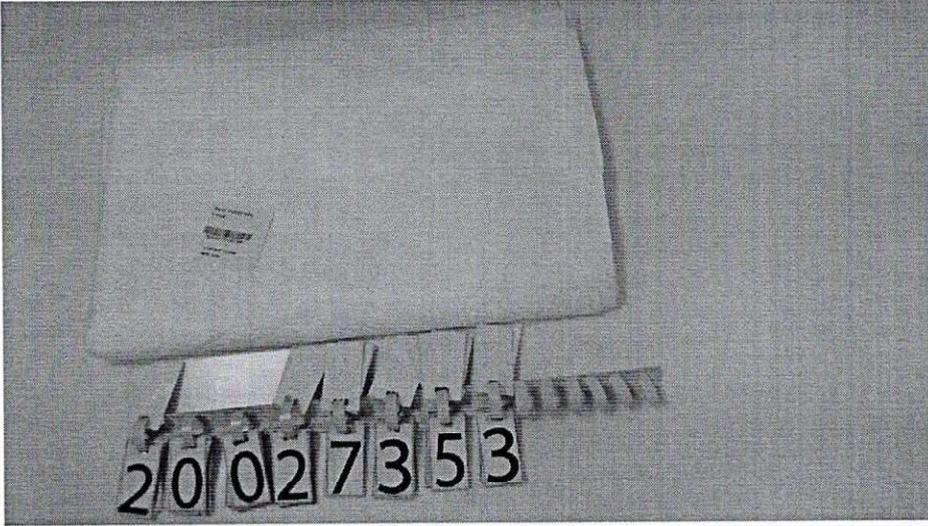

Gen.fl136-2/03

This report shall not be reproduced other than in full except with the permission of the laboratory.
Testing reports without signature and seal are not valid.

**EKOTEKS LABORATUVAR ve GÖZETİM
HİZMETLERİ A.Ş.**

AB-0583-T

20027353

08-20

TEST RESULTS

WATER RESISTANCE-IMPACT PENETRATION TEST; AATCC 42:2017

Test samples were conditioned for at least 4 hours prior to testing ($65 \pm 5\%$ RH, $21 \pm 2^\circ\text{C}$).

Water temperature : $27 \pm 1^\circ\text{C}$

Amount of sprayed water: 500 ml

	<u>RESULT</u>	<u>REQUIREMENT</u>
Water penetration (g)	0 g	$\leq 1,0$ g (Level 3)

WATER PERMEABILITY; AATCC 127:2017-OPTION 2

Hydrostatic Head Tester, Textest marka Fx 3000 model

Temperature of water 20°C . Pressure increase ratio 10 mbar/dk.

Performed in the conditioned room ($21 \pm 2^\circ\text{C}$ - $65\% \pm 5$)

	<u>RESULT</u>	<u>REQUIREMENT</u>
Sample 1	336.6 cm SS	≥ 50 cmSS (Level 3)
Sample 2	227.5 cm SS	
Sample 3	259.1 cm SS	
Average	274.4 cm SS	

Gen.fl136-2/03